



MISSOURI DEPARTMENT OF HEALTH
STATE PUBLIC HEALTH LABORATORY
DATAMASTER MAINTENANCE REPORT

BREATH ALCOHOL PROGRAM

Complete this report in duplicate at the time of the regular monthly preventive maintenance check, and whenever instrument is repaired. Send copy to Department of Health; retain original in department file.

DATAMASTER SN

201305

DHSS STATE

DATE OF INSPECTION

6-2-09

LOCATION OF INSTRUMENT (STREET AND CITY)

1000 N. BOONVILLE, SPRINGFIELD MO 65802

TIME OF INSPECTION

1212

CHECKLIST: Place a check (✓) to the left of each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unchecked items must be corrected before using instrument.

☒ DIAGNOSTIC CHECK (PRINTOUT ATTACHED)

☒ COMPUTER

☒ DETECTOR

☒ PROGRAM

☒ FILTERS

☒ HEATERS SAMPLE CHAMBER 48 °C

☒ QUARTZ STANDARD

☒ FLOW DETECTOR

☒ CALIBRATION

☒ PUMP HIGH SPEED

☒ PRINTER

☒ INDICATOR LIGHTS

☒ TIME AND DATE

1212 / 6-2-09

☒ SIMULATOR TEMPERATURE (34 °C ± 0.2 °C)

34 °C

☒ CALIBRATION CHECK -

Run three tests using a standard solution. All three tests must be within ± 5% of the standard value and must have a spread of .005 or less. Check the box corresponding to the standard solution being used. (PRINTOUT ATTACHED) (USE RECIRCULATION PUMP)

☒ 0.100% STANDARD - MUST READ BETWEEN 0.095% and 0.105% INCLUSIVE

☐ 0.040% STANDARD - MUST READ BETWEEN 0.038% and 0.042% INCLUSIVE

(ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)

TEST 1 ☒ .099%

TEST 2 ☒ .099%

TEST 3 ☒ .099%

☒ PERFORM R.F.I. TEST (PRINTOUT ATTACHED)

☒ NUMBER OF REFUSALS, SINCE LAST MAINTENANCE REPORT, AND NUMBER OF BREATH TESTS IN EACH RANGE AS FOLLOWS: (DO NOT INCLUDE SIMULATOR TESTS)

REFUSALS 19 (0-.04) 4 (.05-.09) 7 (.10-.14) 26 (.15-.19) 15 (Over .19) 10

List any new parts and describe any alteration or modification that was made to restore the instrument to operate satisfactorily and within established limits (use other side if necessary)

MEETS ALL MOH STANDARDS, REPCO 100% SOLUTION
LOT # 08002, EXPIRES 10-13-2010

INSPECTING OFFICER

SIGNATURE

PRINT NAME

TYPE # PERMIT NUMBER/EXPIRATION DATE

TELEPHONE NUMBER

820216 / 7-23-10

SHAWN CRAWSON
(417) 864-1810

CERTIFICATE OF ANALYSIS


Random samples of lot number 08002 of Alcohol Certified Solution for simulator were analyzed by an independent laboratory utilizing a gas chromatograph and found to contain .1209 gms/dl wt. /vol. ethyl alcohol.

The alcohol and distilled water used in the solution were found to be free of any interfering substance.

When used in a calibrated simulator, operating at 34 c +/- .2 c, this solution will give an alcohol breath test instrument reading of .100 percent BAC +/- 2% or .002 BAC (whichever is greater).

The expiration date for this lot number is October 13, 2010 at 11:59PM.

This document is a true representation of the original Certificate of Analysis.

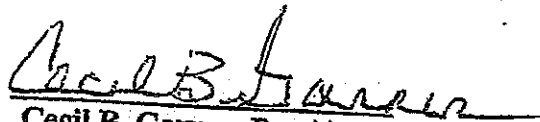
Cecil B. Garner, President
RepCo Marketing, Inc.

Face This Side Down - This Edge In First

BAC DataMaster Evidence Ticket

SPRINGFIELD POLICE DEPT
BAC DATAMASTER SERIAL NUMBER 281305
06/02/09
12:12

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
HEATERS
SAMPLE CHAMBER: 48c
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJ
KLMNOPQRSTUVWXYZ[\]^_`abdefghijklmnop
qrstuvwxyz{|}~

Operator Signature

Face This Side Down - This Edge In First

BAC DataMaster Evidence Ticket

SPRINGFIELD POLICE DEPT
BAC DATAMASTER SERIAL NUMBER 281305
06/02/09

TESTING OFFICER:

CLAWSON

OFFICER I.D.: 1226

PERMIT NUMBER: 820216

EXPIRATION DATE: 07/23/10

MISCELLANEOUS DATA:

CAL CHECK

--- SUPERVISOR MODE ---

BLANK TEST	.000	12:12
INTERNAL STANDARD	VERIFIED	12:13
EXTERNAL STANDARD	.099	12:14
BLANK TEST	.000	12:14
EXTERNAL STANDARD	.099	12:15
BLANK TEST	.000	12:15
EXTERNAL STANDARD	.099	12:16
BLANK TEST	.000	12:16

N = 3

SIM. = .1

AVG. = .099

Operator Signature

Face This Side Down - This Edge In First

BAC DataMaster
Evidence Ticket

SPRINGFIELD POLICE DEPT
BAC DATAMASTER SERIAL NUMBER 201305
06/02/09

ARREST TIME: 11:00

SUBJECT NAME:

RFI/TEST

DOB: 11/11/11 SEX: M

STATE/D.L.: MO/123456789

ARRESTING OFFICER:

CLAWSON

OFFICER I.D.: 1226

TESTING OFFICER:

CLAWSON

OFFICER I.D.: 1226

PERMIT NUMBER: 820216

EXPIRATION DATE: 07/23/10


MISCELLANEOUS DATA:

RFI TEST

--- BREATH ANALYSIS ---


RADIO INTERFERENCE

Operator Signature




2208-02

State of Missouri
DEPARTMENT OF HEALTH



P E R M I T
TYPE II



SHAWN CLAWSON

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field repairs, and operate the following breath analyzer(s):

DATAMASTER;INTOXILYZER 5000

for the determination of the alcoholic content of blood from a sample of expired (alveolar) air. Issued under the provisions of sections 577.020 through 577.041, RSMo 1986.

07/23/08

Date

820216

Number

07/23/2010

Expires

MO 580-0771 (7-88)

Director of State Public Health Laboratory

W. E. B. B. B.

Director, Department of Health

Lab. 4 (R7-88)